

Tens FM-B2409



Pain Relief, Anywhere, Anytime.

Please read the instructions manual carefully before using the device.



Manufacturer: SHENZHEN JIANFENG ELECTRONIC TECHNOLOGY CO; LTD. Address: #902,903 JIALINGYU INDUSTRIAL BUILDING, DA PU ROAD, HOUTING VILLAGE, SHAJING TOWN, BAOAN DISTRICT,SHENZHEN, GUANGDONG,CHINA 518100

Customer Service:

Support@belifu.com Please download the PDF manual on the below link: https://belifu.com/downloads/

Precaution

Please read the instructions manual carefully before using the device.

If you have any questions, please refer to the salesman or ask your doctor.

Please keep this manual for future reference.

CONTENT

- Chapter 1 : Introductions
- Chapter 2 : Functions Of The Device
- Chapter 3 : Warnings And Notes
- Chapter 4 : Operation
- Chapter 5 : Battery And Memory Function
- Chapter 6 : Maintenance
- Chapter 7 : Mode Instruction
- Chapter 8 : TENS EMS Electrode Placement Guide
- Chapter 9 : Troubleshooting
- Chapter 10 : Product Descriptions
- Chapter 11 : Medical Disclaimer
- Chapter 12 : Precautions
- Chapter 13 : Contraindications
- Chapter 14 : Adverse Reaction
- Chapter 15 : Notes On FCC Certification
- Chapter 16 : Warranty

Chapter 1: Introductions

Working principle

It acts on the human body through the electricity pulse wave, the electric energy is sucked by the human body and the energy form is changed, which causes a series of physical and chemical changes, produces local or systemic physiological reactions, and finally affects the pathological process and plays a corresponding role.

Intended use

For TENS mode: To be used for temporary relief of pain and recovery of fatigue associated with sore and aching muscles due to strain from exercise or normal household work activities.

For EMS mode: To be used to stimulate healthy muscles in order to improve and facilitate muscle performance.

Applicable people

Adults who suffer from sore and aching muscles in the shoulder, waist, back, neck, upper extremities (arms), and lower extremities (leg) due to strain from exercise or normal household work activities can use this device.

However, it should not be used by children, pregnant women, or anyone who has an implanted metallic or electronic device. Ask your physician if you have any questions.


Package list

- Device
- ·1 pair of large self-adhesive electrode pads
- ·3 pairs of medium self-adhesive electrode pads
- ·1 pair of small self-adhesive electrode pads
- ·2 lead wires with 2 connectors (2.5mm)
- ·USB cable
- Storage bag
- ·User manual

Features

- ·36 modes
- ·20 intensity levels
- ·Type-C Rechargeable lithium battery
- ·20-minute default timer, adjustable from 10-80 minutes or continuously

Chapter 2: Functions Of The Device

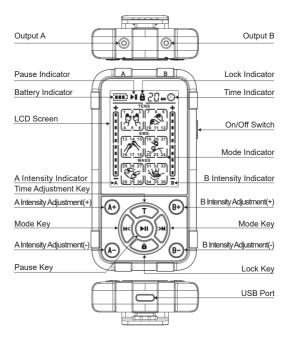

Chapter 3: Warnings And Notes

Warnings

We recommend not to use this therapeutic apparatus in the following cases:

- Do not use this device if the patient has any implantable electronic or metal equipment (e. g. pacemaker).
- 2) Has epilepsy.
- Severe lower extremity arterial circulation problems.
- 4) Abdominal or inguinal hernia site.
- Do not use this device if you have a heart disease without consulting a doctor.
- Do not use this device on pregnant women.
- Do not use this device over, or in proximity to, cancerous lesions.
- 8) Be Fever.
- 9) Has cancer.
- Do not use therapeutic instruments in high humidity environments, such as bathing or showering in a bathroom bathtub.
- 11) Can not be used after drinking.

- 12) Low-frequency therapeutic instruments can not be used when using high-frequency surgical instruments.
- 13) Near the genitals.
- 14) Recommendation: do not use low-frequency therapeutic instruments near shortwave or microwave therapeutic equipment (e. g. 1m), where the output of the low frequency therapeutic instrument used is unstable.
- 15) The high frequency surgical equipment and stimulator. When connected to a patient, burns may occur at the stimulator electrode and may damage the stimulator.
- 16) Patients undergoing medical treatment and feeling abnormal.
- 17) Heart patients with neurological abnormalities in the brain.
- Patients whose body temperature exceeds 38 °C .
- 19) Infectious diseases Patients.
- 20) Patients who can not express their will.
- 21) Do not use this product while charging.

Notes

- Electrode wire is too long may cause suffocation. Keep the product and keep away from children.
- Make sure you are always aware of all warning items.
- 3) Stimulators should not be used in the throat and mouth. This may result in severe throat muscle spasms and muscle contraction, which is sufficient to block the airway and cause dyspnea.
- The application of electrodes near the thorax may increase the risk of cardiac fibrillation
- 5) This stimulator should not treat unattended patients, or suffer from emotional distress, dementia, and low IQ people.
- 6) Use guidance has been detailed; any improper use may lead to danger.
- Do not use this device for any undiagnosed pain symptoms, consult a doctor for diagnosis before use.
- 8) Electrodes can not be placed in arteries, head and pubic area.
- 9) Patients suffering from heart disease, cancer or other health-threatening conditions should consult a doctor before using this device.

- 10) If the intensity of stimulation makes you feel 8 uncomfortable, reduce the intensity of stimulation to a comfortable level. If the problem remains, please contact your doctor.
- Do not use this equipment in rooms where aerosol (spray) and pure oxygen are used.
- Please do not use this equipment near any highly flammable substances, gases or explosives.
- Please check that the cable and related connections are in good condition before each use.
- 14) Turn off the device before using or removing the electrode pad.
- Electronic stimulator can only use electrode wires and electrodes recommended by manufacturers.

Consult your doctor before using the device especially in the following cases:

- Acute disease, especially patients suspected or suffering from hypertension, thrombosis or malignant mass.
- Patients with various skin diseases.
- Patients with chronic pain disorders

(e. g. metabolic disorders) with reduced pain.

• Patients undergoing medication.

Adverse reaction

- Skin allergies caused by electrode sheetpad gels and electrode irritation burns are potential adverse reactions. If the skin appears sensitive response, should be discontinued and consult your doctor.
- If the intensity of stimulation makes you feel uncomfortable, reduce the intensity of stimulation to a comfortable level, and if the problem persists, please contact your doctor.

Explanation of figures. symbols, warning statements and abbreviations on the equipment

| Meanings of symbols used for marking described in instructions for use | | |
|---|---|--|
| $\overline{\mathbb{V}}$ | Caution! | |
| Ŕ | Type BF applied part | |
| ==== | Direct current | |
| IP22 | Protected against solid foreign objects of 12,5mm Φ and greater; Protection against vertically falling water drops when ENCLOSURE tilted up to 15° | |
| \$ | Refer to instruction manual | |
| SN | Serial Number | |
| M | Manufacture date | |
| | Manufacture information | |

Chapter 4: Operation

Before using the device, please check following carefully:

- 1. Check the pads for any damages or irregularities
- 2. Check the electrode wires for any damages or irregularities
- 3. Check the electrode pads any damages or irregularities
- 4. Check for any physical damage on the unit

▲ NOTE: Do not use this product while charging.

STEP 1: Connect the electrode pads to the electrode wires

Note: Please check the snap connections to ensure they are fastened. Use at least one pair of pads, one pads can't work alone.

STEP 2: Plug the wires into the port at the top of the unit

Note: Please make sure the wires are fully inserted to the end. Make

sure the wires are not loose. A loose connection will decrease the power of the output.

STEP 3: Paste the pads on your skin

Note: When using 1 wire with 2 connectors please make sure both pads are stuck on your body; when using 2 wires, please make sure at least 2 pairs of pads are stuck on your body. Please confirm the wire is plugged well and pads are stuck to your skin before adjusting the unit.

Note: When the electrode pad is stuck to the clothes, don't tear it off heavily. As long as the inside of the side with the electrode pad is covered with water, it can be removed easily.

STEP 4: Turn on the unit

Long press the "Power" button located on the right side of the unit to turn on the device. The screen will light up.

Note: Please check the flash channel indicator on the screen to make sure it is the channel you want to use. The flash "A" icon indicates you can adjust the mode and intensity level of Channel A. If you choose Channel B, the Channel B icon will flash to indicate the Channel B is working.

STEP 5: Choose the channel

The default value is Channel A. Please press the "**A+**" or "**B+**" key to choose the channel you want to use, then the selected **A** or **B** icon on screen will flash.

Note: The channel is independent, you can set different mode and intensity on different channel. Please confirm the channel you want to use before choosing the mode and intensity

STEP 6: Choose the mode and adjust the intensity

- Press the "M<" or ">M" key to select one main mode. The selected mode and number will flash. (Note: There are two options to select modes: 1. You can select the mode directly when long press the "M<" or ">M" button. The mode icon will keep bouncing in a continuous cycle until your hand release from the mode button 2. Short press the "M<" or ">M" button, the mode will be selected one by one)
- 2.Press the "A+" "A-"or "B+" "B-"keý to increase or decrease the intensity level. The treatment will start when the intensity is higher than 0.

Note: Remember the strength will default to the 0 when changing the mode. It is recommended to start with the lowest level of intensity and gradually increase to a level that is comfortable.

STEP 7: Set the time

The default time is 20mins. Press the "T" button to adjust the time (10-80 mins), it can be increased by 10mins. When it's increased up to 80mins, continue to press the "T" button to jump to 10mins.

STEP 8: Pause the treatment

Press the "►II" button to suspend the treatment when changing the massage point, the ►II icon will appear on the s creen, anything setting can't be change in a pause state. Press the "PAUSE" button again to continue treatment.

STEP 9: Lock the device

You can press the " $\mathbf{\hat{e}}$ " button to lock the device to avoid accidental press. The $\mathbf{\hat{e}}$ icon will appear on the screen in locked state. Press the " $\mathbf{\hat{e}}$ " button to unlock the device.

Note: The back light will be off automatically after 30 seconds of inactivity, you can also press the any button to light up or off the screen as you like.

STEP 10: Turn off the device

Long press the "Power" button located on the right side of the unit to turn off the device. The device will automatically turns off when the time runs out.

STEP 11: Remove the pads from your skin and store the products

Remove the pads from you skin gently, and paste the plastic dust-proof film on them, take them off the electrode wires and unplug the wires, put them and the device into the storage bag.

Note: Please don't tear off the pads vigorously. Please don't remove the pad before turning off the device.

Chapter 5: Battery And Memory Function

·Battery information

Please use the AC adapter complying the standard : IEC60601-1, DC5V/500mA) Capacity: 180mAh Voltage: 3.7V

·Charging the battery

- The device is powered by an internal, rechargeable lithium battery that can be charged through a standard wall outlet or through the USB port of a computer or power bank. Signs the device needs to be charged include dimness of the screen or failure to display the screen, and weak sensations from the electrodes.
- 2.Turn off the device.
- 3.Connect the controller and the charger with USB extension cord.Plug charger into any power outlet. The charging process will last 1-2 hours.

Memory function

The memory function can help to remember the selected mode, the Mode will always be the same as the value as before pause and shut down.

Chapter 6: Maintenance

Please clean the main machine frequently. Use a piece of soft dry cloth to wipe the dirt on the main machine. Don't wash with water or clean with the detergent, thinner, volatile oil, etc. that contains chemical substances. The gel surface of the massage pad should be kept clean and avoid dirt like dust, oily substances, sticky substances, etc., otherwise the stickiness will be decreased. Please put the massage pads back to the pad holders or paste the protective films back onto the pads after use. When the stickiness of the massage pad becomes weak due to dirt or if there is a tingling sensation in the skin, please use a piece of damp cloth dipped in a little water to gently wipe the gel surface. After drying, t he stickiness will recover, but if water is overused, the stickiness will be decreased. Please don't wipe the gel surface with a paper towel. Please do not scrape the gel surface with nail, brush, etc. Massage pads are consumables with the

service life of generally 20-30 times. If the pads are not sticky or the pulse becomes weak, please change the pads in time. The batteries for this product are built-in polymer batteries. If it is not used for a long time, please charge it every 6 months.

Safekeeping

Please do not put the main machine in the place exposed to sunlight, high temperature, humidity, lots of dust, or the place close to fire, easy to vibrate or shock.Please put where children can't reach it.

Cleaning and storing pad

Clean: After using pads on your body, please drop a little clean water on the sticky side and use fingertips to clean it softly

- Please turn off the device and disconnect the pads with wires first before you clean the pad.
- Do not use nails or other sharp objects on the sticky side.Do not use chemical liquids on sticky side.

Storage: Place pads on pad holder or place plastic film on the sticky side of pad to keep the gel moisture.

- Do not keep device in areas subject to direct sunlight, high or low temperatures, humid area, near to fire, vibration, or shock.
- Do not keep the device at places that can be easily reached by children.

WARM TIPS FOR SKINCARE

To avoid skin irritation, especially if you have sensitive skin, follow these suggestions:

- Wash the area of skin where you will be placing the electrodes, using mild soap and water before applying electrodes, and after taking them off. Be sure to rinse soap off thoroughly and dry skin well.
- 2. Excess hair may be clipped with scissors; do not shave stimulation area.
- 3. Wipe the area with skin preparation wipes. Let the area dry.Apply electrodes as directed.
- 4. Many skin problems arise from the "pulling stress" from adhesive patches that are excessively stretched across the skin during application. To prevent this, apply electrodes from centre outward; avoid stretching over the skin.5. To minimize "pulling stress", tape extra lengths of lead wires to the skin in a loop to prevent tugging on electrodes.
- When removing electrodes, always remove by pulling in the direction of hair growth.
- It may be helpful to rub skin lotion on electrode placement area when not wearing electrodes.
- 8. Never apply electrodes over irritated or broken skin.

Chapter 7: Mode Instruction

Modes & Functions

| Main Mode 1: Tui na | Modes 1~6 | Simulation of Tuina is a hands-on body treatment which help with muscle pain relief and relaxation. |
|------------------------------------|----------------|---|
| Main Mode 2: Acupun cture | Modes 7~12 | Simulation of acupuncture provides the same sensation without needles, by utilizing electronic pulses to achieve the sensation of differing needle depths. |
| Main Mode 3: Tapping | Modes 13~18 | Stimulating tapping is intended to produce a hard thumping sensation that massages your muscles, which can give you an invigorat- ed and revitalized feeling. |


| Main Mode 4: Cupping | 19 20 21 22 23 24 | Modes 19~24 | Mimic the sensation of suction created on the skin. Cupping is a traditional Chinese therapy in which heated glass cups are applied to the skin, creating suction as a way of stimulating the flow of energy. |
|-------------------------------------|----------------------|----------------|--|
| Main Mode 5: Scraping | 25 26 27 28 29 30 | Modes 25~30 | Stimulate pain points in the elbow area for pain relief or muscle relaxation. |
| Main Mode 6: Combin- ation | 31 32 33 34 35 36 | Modes 30~36 | Deep tissue massage therapy is similar to Swedish massage, but the keeper pressure is beneficial in releasing chronic muscle tension. |

Chapter 8: TENS EMS Electrode Placement Guide

For TENS



For EMS

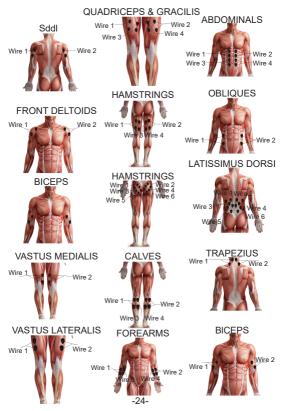

Chapter 9: Troubleshooting

| Problems | Causes | Solutions |
|--|---|---|
| Adhesive gel pads are not adhering firmly to the skin. The gel pads are too dry. | Adhesive gel pads are not adhering firmly to the skin. The gel pads are too dry. | Apply a few drops of water to the adhesive surface of each pad and make sure the pads are pressed firmly to the skin during application |
| Skin feels a painful burning sensation, or the stimulation becomes weakened. | Adhesive gel pads are not adhering firmly to the skin. The gel pads are too dry. | Apply a few drops of water to the adhesive surface of each pad and make sure the pads are pressed firmly to the skin during application |
| Unit is on, but no sensation is felt from the pads. | Both pads are not firmly on the skin. There is a loose connection. The intensity level needs to be increased. | Make sure all pads are firmly pressed to the skin. Make sure all connections are well from the unit to the wires and the wires to the pads. Increase the intensity level. |
| Adhesive gel pads do not stick to skin even after cleaning and moistening the gel pad. | Adhesive gel pads need to be replaced. | Replace the pads. You can contact support@belifu.com to purchase the pads. |
| Unit does not turn on or the screen is dim. | Battery is low. | Recharge the battery. |
| Does not provide adequate pain relief. | Not using it long enough. | Use your massager 20-30 minutes at a time, 3-6 times per day. |

| Unit turns on, all of the modes and channels flash. Can not select a mode and adjust the intensity. | Adhesive gel pads are not adhering firmly to the skin.The gel pads are too dry. | Apply a few drops of water to the adhesive surface of each pad and make sure the pads are pressed firmly to the skin during application |
|--|--|--|
| Unit turns on, all of the modes and channels flash. Can not select a mode and adjust the intensity. | Always use two pads (one channel) or four pads (two channels) at the same time as it will not work with just one pad or three pads. | When you use two pads (one channel) or four pads (two channels) at the same time, make sure you have placed all pads on your body, otherwise it won't work. |
| The pluses strong on one side and weak on the other side. | Different nerve distribution in different parts of the body, different skin sensitivity, or insufficient skin contact with the electrodes. | Please wipe the skin with a wet towel before use to ensure adequate contact with the electrode. It suggested that the two electrodes should be sym metrical when attached to the body |
| Key failure | The machine is locked or paused. | Press the "LOCK" key to unlock the device or press the "PAUSE" key to continue the treatment. |
| Feeling unwell | Too strong. Too close between electrodes. | Electrodes or conductors are damaged. The electrode area is too small. Decrease intensity Reorient electrode position. Replace the electrode wire or pads. |

Chapter 10: Product Descriptions

| Product name | TENS & EMS Device |
|--------------------------------------|-----------------------------|
| Model | FM-B2409 |
| Charge time | About 2 hours |
| Battery run time | About 8 hours |
| Lithium battery power supply | 3.7V/180mAh |
| Load resistance | 500Ω |
| Output frequency | 0Hz~199Hz |
| Maximum pulse width | 220uS |
| Low voltage protection | MAX≤3.3V |
| Weight | 55.3g |
| Size | 100mm*54mm*15mm |
| Number of channels | 2 |
| Treatment time | 10-80mins |
| AC adapter | 110V-240V |
| Charging interface | TYPE-C USB |
| Backlight current | 20-30mA |
| Operating current | 0~60mA |
| Standby current | 0~10mA |
| Quiescent current | 0∼5uA |
| Display | LCD liquid crystal |
| Operating environment temperature | 5°C ~40°C (41.0 °F ~104 °F) |
| Battery capacity | 180mAh 27- |

Chapter 11: Medical Disclaimer

All information is intended for you general knowledge only and is not a substitute for medical advice or treatment for specific medical conditions. We cannot and do not give you medical advice. You should seek prompt medical care for any specific health issues and consult your health care provider before purchasing any product(s). The information contained here is intended to provide broad consumer understanding and knowledge of product offered.

The information should not be considered complete and should not be used in place of a visit, call, consultation or advice or your health care provider. Should you have any healthcare-related questions, please call or see your health-care provider promptly. You should never disregard medical advice or delay in seeking it because of something you have read here.

Precautions to be taken in the event of changes in the performance of me equipment or me system

Me equipment, me systems and accessories require professional hygienic maintenance prior to re-use. When the ME equipment is transferred to another patient, please contact us for the relevant service.

Disposal Information

Please contact the local authorities to determine the proper method of disposal of the used equipment and accessories.

Chapter 12: Precautions

- 1.Safety of this device for use during pregnancy has not been established.
- Caution should be used for patients with suspected or diagnosed heart problems.
- 3.Caution should be used for patients with suspected or diagnosed epilepsy.
- 4.Caution should be used in the presence of the following:
- •When there is a tendency to hemorrhage following acute trauma or fracture;
- Following recent surgical procedures when muscle contraction may disrupt the healing process;
- •Over the menstruating or pregnant uterus;
- •Over areas of the skin which lack normal sensation.
- 5.Some patients may experience skin irritation or hypersensitivity due to the electrical stimulation or electrical conductive medium. The irritation can usually be reduced by using an alternate conductive medium, or alternate electrode placement.
- 6.Electrode placement and stimulation settings should be based on the guidance of the prescribing practitioner.

- 7. The device should be kept out of the reach of children.
- The device should be used only with the leads and electrodes recommended for.
- 9. This device should not be used while driving, operating machinery, or during any activity in which involuntary muscle contractions may put the user at undue risk of injury.

Chapter 13: Contraindications

Do not use this device if you have an implanted electronic device, i.e. a cardiac pacemaker, implanted defibrillator, or other implanted metallic or electronic device unless specialist medical opinion has first been obtained. Such use could cause electric shock, burns, electrical interference, or death.

Chapter 14: Adverse Reaction

- •Skin irritation and burns beneath the stimulation electrodes applied to your skin.
- •Headache and other painful sensations during or following the application of electrical stimulation near your eyes, to your head and face.
- Potential allergic reactions due to the electrical stimulation or gel including: skin irritation, redness, burning or hypersensitivity.

*** You should stop using the device and consult with your physician if you experience any adverse reactions from the device. ***

Potential Electromagnetic and Other Interference

This product is sensitive to the electromagnetic interference, and the following cases may interfere with normal use: •When talking on the mobile phone; •Near the base station for signal transmission (broadcast, television, communications, radar, navigation. etc.): Near high radiation medical instruments such as nuclear magnetic resonance; The operator should be away from the equipment or occasion as soon as possible if the essential performance of the equipment is degraded or lost due to EM DISTRUBANCES. The essential performance of the equipment should be restored. If not, please contact your seller.

Chapter 15: Notes On FCC Certification

This device has been tested and found to comply with the limits for a Class B digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This device generates uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this device does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures:

- Reorient or relocate the receiving antenna.
- Increase the separation between the equipment and receiver.
- Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.
- Consult the dealer or an experienced for help.
- Consult the seller or **support@belifu.com** for help.

Any Changes or modifications not expressly approved by the party responsible for compliance could void the user's authority to operate the device.

Chapter 16: Warranty

- The warranty period for device is two year from date of delivery. In case of a warranty claim, the date of delivery has to be proven by means of the sales receipt or invoice.
- 2) Repairs under warranty do not extend the warranty period.
- The following cases are not included in the warranty.
- All damage which has arisen due to improper treatment, e.g. nonobservance of the user instruction.
- All damage which is due to repairs or tampering by the customer or unauthorized third parities.
- Damage which has arisen during transport from the manufacturer to the consumer or during transport to the service centre.
- Accessories which are subject to normal wear and tear.
- 4) Liability for direct or indirect consequential losses caused by the unit is excluded even if the damage to the unit is accepted as a warranty claim.
- 5) Anything about the device, please feel free to contact **support@belifu.com**